



[1] **EU-TYPE EXAMINATION CERTIFICATE - Translation**

[2] Equipment or protective systems
intended for use in potentially explosive atmospheres, Directive 2014/34/EU

[3] EU-type examination certificate number **IBExU10ATEX1068 X** | Issue 3

[4] Product: **Pressure measuring devices**
Type: DX19-DMP..., DX19-DMK..., DX19-LMP..., DX19-LMK..., DX19-17.600G,
DX19-17.605 and DX19-26.600

[5] Manufacturer: **BD | SENSORS GmbH**

[6] Address: **BD-Sensors-Str. 1
95199 Thierstein
GERMANY**

[7] This product and any acceptable variation thereto is specified in the schedule to this certificate and the documents therein referred to.

[8] IBExU Institut für Sicherheitstechnik GmbH, Notified Body number 0637 in accordance with Article 17 of Directive 2014/34/EU of the European Parliament and of the Council, dated 26 February 2014, certifies that this product has been found to comply with the essential health and safety requirements relating to the design and construction of products intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in the confidential test report IB-24-3-0067.

[9] Compliance with the essential health and safety requirements has been assured by compliance with:
EN IEC 60079-0:2018 and EN 60079-11:2012
except in respect of those requirements listed at item [18] of the schedule.

[10] If the sign "X" is placed after the certificate number, it indicates that the product is subject to the specific conditions of use specified in the schedule to this certificate.

[11] This EU-type examination certificate relates only to the design and construction of the specified product. Further requirements of the Directive apply to the manufacturing process and supply of this product. These are not covered by this certificate.

[12] The marking of the product shall include the one of the following depending on the used components:

Non-metallic pressure connection II 2 G Ex ia IIC T4 Gb (type *457* only IIB)
 II 2 D Ex ia IIIC T85 °C Db

Metallic pressure connection II 1 G Ex ia IIC T4 Ga (type *457* only IIB)
 II 1 D Ex ia IIIC T135 °C Da or
 II 2 D Ex ia IIIC T85 °C Db

IBExU Institut für Sicherheitstechnik GmbH
Fuchsmühlenweg 7
09599 Freiberg, GERMANY

Tel: + 49 (0) 37 31 / 38 05 0
Fax: + 49 (0) 37 31 / 38 05 10

By order

Dr.-Ing. P. Cimalla



Certificates without signature and seal are not valid. Certificates may only be duplicated completely and unchanged. In case of dispute, the German text shall prevail.

Freiberg, 2024-11-22

[13]

Schedule

[14]

Certificate number IBExU10ATEX1068 X | Issue 3


[15]

Description of product

The Pressure measuring devices DX19 are different pressure transmitters or level sonde in stainless steel enclosure with different pressure ports. As measuring cell and evaluation electronic serves separately approved electronic modules. The devices are intended for use in potentially hazardous areas, where Category 1 G, 1 D or 2 G, 2 D devices are required. They are supplied by an intrinsically safe power supply of the Category „ia“.

Type code:

DX19- D M P nnn I

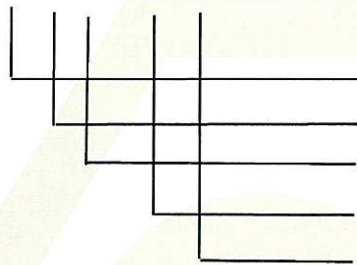

D - pressure measurement devices; L – level sonde

M - transmitter

P – stainless steel cell; K - ceramic cell

nnn - design

I - precision; P - process pressure port

Exceptions: DMK457 KRO
 17.600G, 17.605G, 26.600G

with EMV 45 as clamp platine
conform to DMP

Type extent:

Name	Type	Electronic module	Measurement cell
DMP 311	DMU	ELMO-STA ELV 68 with EMV 26	DSP4XX. ICS86, NPI15 with ELV 66, ELV 70, ELV 86
DMP 321	DMU	ELMO-PRE ELI 37 with EMV 52	DSP4XX, ICS86, NPI15, ST1 with ELV 79, ELV 67, ELI 68, ELI 69, ELI 57, ELI 63, ELI 73
DMP 321 P	DMU	ELMO-PRE ELI 37 with EMV 52	DSP4XX, ICS86, NPI15, ST1 with ELV 79, ELV 67, ELI 68, ELI 69, ELI 57, ELI 63, ELI 73
DMP 321 PT	DMU	ELMO-PRE ELI 93 with EMV 52 PD 79	DSP4XX, ICS86, NPI15, ST1 with ELV 79, ELV 67, ELI 68, ELI 69, ELI 57, ELI 63, ELI 73
DMP 331	DMU	ELMO-STA	DSP 4XX / ELV 66 = DSP 4XX Z alternative ICS 86 / ELV 70 = ICS 86 Z
DMP 331 P	DMU	ELMO-STA	DSP 4XX / ELV66 = DSP 4XX Z alternative DSP 1XX / ELV66 = DSP 1XX Z
DMP 331 Pi	DMU	ELMO-PRE ELI 37 with EMV 52	DSPX21 UM / DSPX21 US DSPX21 UH
DMP 333	DMU	ELMO-STA	DSP 4XX / ELV 66 = DSP 4XX Z alternative NPI 15
DMP 333 P	DMU	ELMO-PRE ELI 37 with EMV 52	DSPX14 UM / DSPX14 US DSPX14 UH
DMP 334	DMU	ELMO-STA ELV 68 with EMV 26 or ELV 93 with EMV 65	ST1 with ELV 97
DMP 334 i	DMU	ELMO-PRE ELI 37 with EMV 52	ST1 with ELI 188
DMP 335	DMU	ELMO-STA	MSP12X / ELV 57 = MSP12X Z alternative PSP 8 / PSP 10 / ELV 135
DMP 336	DMU	ELMO-STA ELV 133	PSP 8

Name	Type	Electronic module	Measurement cell
DMP 339	DMU	ELMO-STA ELMO-PRE	ICS 89 / ELV 66 / ELV 68 / EMV 26 ICS 89 / ELI 36 / ELI 37 / EMV 52
DMP 339 P	DMU	ELMO-PRE ELI37 mit EMV 52	PSP 8 PD 98 / ELI 101
DMP 343	DMU	ELMO-STA	DSP 210 / ELV 66 = DSP 210 Z
DMP 457	DMU	ELMO-STA	DSP 4XX / ELV66 = DSP 4XX Z alternative ICS 86 / ELV 70 = ICS 86 Z EMV 58 replaces EMV 26 from ELMO-STA
17.600G	DMU	ELMO-STA	MSP12X / ELV57 = MSP12X Z alternative PSP 8 / PSP 10 / ELV 135
17.605G	DMU	ELMO-STA	SPS 1000 / ELV 49 / ELV 68 / EMV 26
26.600G	DMU	ELMO-STA	DSK611 / ELV 49 / ELV 68 / EMV 26
DMK 331	DMU	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z
DMK 331 P	DMU	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z
DMK 331	DMU	ELMO-STA ELV 68 with EMV 26 or ELV 93 with EMV 65	DSK 516 with ELV 94
DMK 457	DMU	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z EMV 58 replaces EMV 26 from ELMO-STA
DMK457 KRO	DMU	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z additional with EMV 45 as clamp platine.
DMP 331 i	DMU	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative ICS 86 / ELI 20 with aid platine PD 16
DMP 333 i	DMU	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative NPI 15
LMP 307 ¹	PS	ELMO-STA	DSP 4XX / ELV66 = DSP 4XX Z alternative ICS 86 / ELV 70 = ICS 86 Z
LMP 308	PS	ELMO-STA	DSP 4XX / ELV66 = DSP 4XX Z alternative ICS 86 / ELV 70 = ICS 86 Z
LMP 331	DMU	ELMO-STA	DSP 4XX / ELV66 = DSP 4XX Z alternative ICS 86 / ELV 70 = ICS 86 Z
LMK 307	PS	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z
LMK 331	PS	ELMO-STA	DSK 511 / ELV 58 = DSK 511 Z
LMP 307 ²	PS	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative ICS 86 / ELI 20 with aid platine PD 16
LMP 307 i	PS	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative ICS 86 / ELI 20 with aid platine PD 16
LMP 308 i	PS	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative ICS 86 / ELI 20 with aid platine PD 16
LMP 331 i	PS	ELMO-PRE ELI 103 – ELI 121	DSP 4XX / ELI 20 = DSP 4XX X alternative ICS 86 / ELI 20 with aid platine PD 16

¹⁾ except for accuracy 0,1 % or accuracies > = 0,25 %

²⁾ for accuracy 0.1 %

Technical Data

Ambient temperature range:

Standard version:

Precision instrument (I):

from -40 ° C / -20 ° C to +70 ° C

from -40 ° C / -20 ° C to +65 ° C

Electrical DataSupply and signal electric circuit
(+ and -)

in type of protection Intrinsic Safety Ex ia IIC

U_i 28 V DCI_i 93 mAP_i 660 mW

effective inner capacity

C_i negligible

effective inner inductivity

L_i negligible

plus line inductivities 1 µH/m and line capacities 160 pF/m (cable supplied by the manufacturer)

For all types except *457*, the supply connections have an internal capacity of max. 27 nF to the housing.

The effective internal capacitance is increased to C_i = 105 nF with the housing type *457* with field housing, with cable output C_i = 84.7 nF and with ISO 4400 C_i = 62.2 nF. The supply connections of these devices have an internal capacitance of max. 90 nF (140 nF with field housing) to the housing.

Variations compared to the issue 2 of this certificate:

Variation 1

Adding of device types DMP 331 Pi, DMP 334 i, DMP 339 P and DMP 333 P.

Variation 2

Adding of cable box GDS 307 from Fa. Hirschmann.

[16] Test report

The test results are recorded in the confidential test report IB-24-3-0067 of 2024-11-15.

The test documents are part of the test report and they are listed there.

Summary of the test results

The pressure measuring devices DX19-DMP..., DX19-DMK..., DX19-LMP..., DX19-LMK..., DX19- 17.600G, DX19-17.605 and DX19-26.600 still fulfil the requirements of type of protection Intrinsically safety 'ia' on an electrical device for Equipment Group II Category 1 G, 2 G, 1 D or 2 D, Explosion Group IIC or IIB and temperature class T4.

[17] Specific conditions of use

- The safety and assembly instructions contained in the operating instruction and the ambient temperature range depending on cable type $-40\text{ °C} / -20\text{ °C} \leq T_a \leq +70\text{ °C}$ or at the types DX19-*** I $-40\text{ °C} / -20\text{ °C} \leq T_a \leq +65\text{ °C}$ have to be taken into account.
- The device may be operated in explosive atmospheres, which require equipment of Category 1 only when there are atmospheric conditions (temperature of -20 °C to $+60\text{ °C}$, pressure of 0.8 bar to 1.1 bar).
- The equipment designed with connector has to be installed in such a way that the degree of protection IP20 is always kept.

[18] Essential health and safety requirements

In addition to the essential health and safety requirements (EHSRs) covered by the standards listed at item [9], the following are considered relevant to this product, and conformity is demonstrated in the test report:

None

[19] Drawings and Documents

The documents are listed in the test report.

IBExU Institut für Sicherheitstechnik GmbH

Fuchsmühlenweg 7

09599 Freiberg, GERMANY

By order

Dr.-Ing. P. Cimalla

Freiberg, 2024-11-22